


Serological Pipettes



Your Trusted Partner in Life Sciences

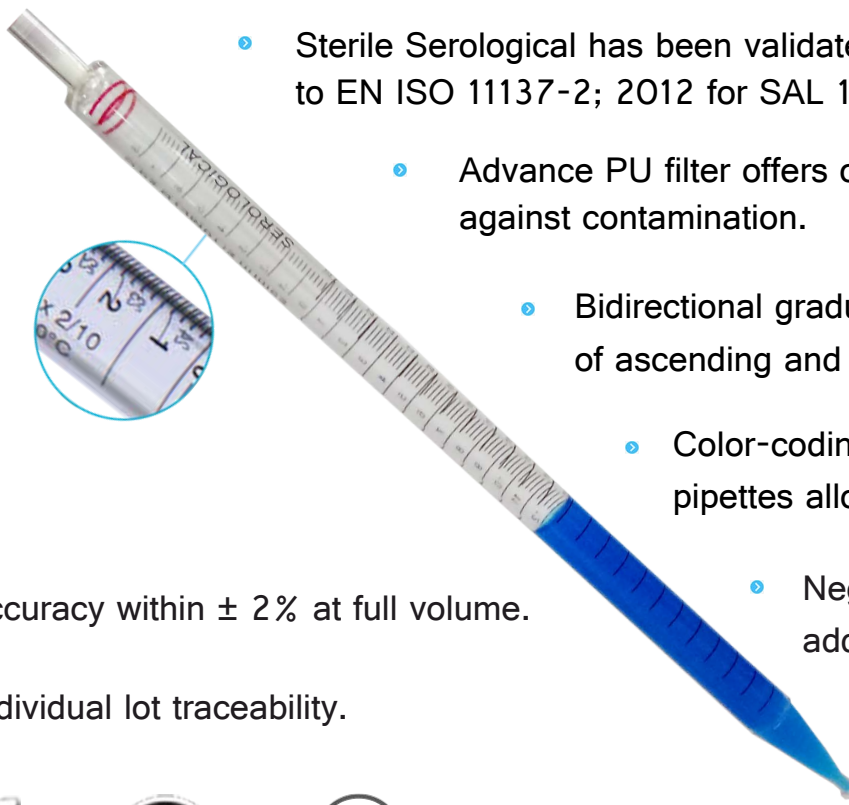

- Sterile Serological has been validated according to EN ISO 11137-2; 2012 for SAL 10⁻⁶.
- Advance PU filter offers complete protection against contamination.
- Bidirectional graduations provide choice of ascending and descending scales.
- Color-coding on paper/serological pipettes allows easy size identification.
- Negative graduations allow additional working volume.
- Accuracy within $\pm 2\%$ at full volume.
- Individual lot traceability.



Cotton plug can be a major source of contamination to your experiment. Abdos advance PU filter offers complete protection against contamination which gives hassle & anxiety free results.

Code	Length (mm)	Capacity (ml)	No. per Case
P10601	270	1	500
P10602	270	2	400
P10603	295	5	200
P10604	295	10	200
P10605	298	25	200
P10606	300	50	100

For additional product or technical information, please visit www.abdoslifesciences.com. For distributor information contact labtech@abdosindia.com.

Abdos Labtech Pvt Ltd

720 - 722, DLF Tower A, Jasola,
New Delhi - 110025, India.

T: +91-11-44800980-986

F: +91-11-44800987

E: labtech@abdosindia.com

Europe Office

T: +44 - 7958295643

E: eu.labtech@abdosindia.com